

X-Series Signal Analyzer 20 Hz to 3.6, 8.4, 13.6, or 26.5 GHz

**Data Sheet** 



### **Table of Contents**

Definitions and Conditions	. 3
requency and Time Specifications	. 4
Amplitude Accuracy and Range Specifications	. 6
Dynamic Range Specifications	. 8
PowerSuite Measurement Specifications	12
General Specifications	13
nputs and Outputs	14
Related Literature	18

### Accelerate to market

Every device demands decisions that require tradeoffs in your goals—customer specs, throughput, yield. With a highly flexible signal analyzer, you can manage and minimize those tradeoffs. Agilent's mid-performance MXA is the ultimate accelerator as your products move from design to the marketplace. It has the flexibility to quickly adapt to your evolving test requirements—today and tomorrow. Maximize your flexibility, and accelerate to market, with the Agilent MXA signal analyzer.

### **Definitions and Conditions**

Specifications describe the performance of parameters covered by the product warranty and apply to the full temperature range of 0 to 55  $^{\circ}$ C  $^{1}$ , unless otherwise noted.

95th percentile values indicate the breadth of the population (approx.  $2~\sigma$ ) of performance tolerances expected to be met in 95 percent of the cases with a 95 percent confidence, for any ambient temperature in the range of 20 to 30 °C. In addition to the statistical observations of a sample of instruments, these values include the effects of the uncertainties of external calibration references. These values are not warranted. These values are updated occasionally if a significant change in the statistically observed behavior of production instruments is observed.

Typical describes additional product performance information that is not covered by the product warranty. It is performance beyond specifications that 80 percent of the units exhibit with a 95 percent confidence level over the temperature range 20 to 30 °C. Typical performance does not include measurement uncertainty.

Nominal values indicate expected performance, or describe product performance that is useful in the application of the product, but are not covered by the product warranty.

The analyzer will meet its specifications when:

- · It is within its calibration cycle
- Under auto couple control, except when Auto Sweep Time Rules = Accy
- Signal frequencies < 10 MHz, with DC coupling applied</li>
- The analyzer has been stored at an ambient temperature within the allowed operating range for at least two hours before being turned on; if it had previously been stored at a temperature range inside the allowed storage range, but outside the allowed operating range
- The analyzer has been turned on at least 30 minutes with Auto Align set to normal, or, if Auto Align is set to off or partial, alignments must have been run recently enough to prevent an Alert message; if the Alert condition is changed from Time and Temperature to one of the disabled duration choices, the analyzer may fail to meet specifications without informing the user

This MXA signal analyzer data sheet is a summary of the complete specifications and conditions, which are available in the MXA Signal Analyzer Specification Guide. The MXA Signal Analyzer Specification Guide can be obtained on the web at:

www.agilent.com/find/mxa manuals

For ordering information, refer to the MXA Signal Analyzer Configuration Guide (5989-4943EN).

For earlier instruments (Serial number prefix < MY/SG/US5051), the full temperature ranges from 5 to 50 °C.

# Frequency and Time Specifications

Frequency rang	ge	DC coupled	AC coupled	
Option 503		20 Hz to 3.6 GHz	10 MHz to 3.6 GHz	
Option 508		20 Hz to 8.4 GHz	10 MHz to 8.4 GHz	
Option 513		20 Hz to 13.6 GHz	10 MHz to 13.6 GHz	
Option 526		20 Hz to 26.5 GHz	10 MHz to 26.5 GHz	
Band	LO multiple (N)			
0	1	20 Hz to 3.6 GHz		
1	1	3.5 to 8.4 GHz		
2	2	8.3 to 13.6 GHz		
3	2	13.5 to 17.1 GHz		
4	4	17 to 26.5 GHz		
Frequency refe	erence			
Accuracy		± [(time since last adjustment x	aging rate) + temperature stability + calibration accuracy]	
Aging rate		Option PFR	Standard	
		± 1 x 10 <sup>-7</sup> / year	± 1 x 10 <sup>-6</sup> / year	
		± 1.5 x 10 <sup>-7</sup> / 2 years		
Temperature stabi	ility	Option PFR	Standard	
20 to 30 °C Full temperature	ranne	± 1.5 x 10 <sup>-8</sup> ± 5 x 10 <sup>-8</sup>	$\pm 2 \times 10^{-6}$ $\pm 2 \times 10^{-6}$	
	calibration accuracy	Option PFR	Standard	
Acinevable initial	canbration accuracy	± 4 x 10 <sup>-8</sup>	± 1.4 x 10 <sup>-6</sup>	
Example frequenc	y reference accuracy	$= \pm (1 \times 1 \times 10^{-7} + 5 \times 10^{-8} + 4)$	x 10 <sup>-8</sup> )	
(with Option PFR)		$= \pm 1.9 \times 10^{-7}$		
1 year after last a	djustment			
Residual FM		* (0.05 H NI)		
Option PFR Standard		$\leq$ (0.25 Hz x N) p-p in 20 ms nominal $\leq$ (10 Hz x N) p-p in 20 ms nominal		
Standard		See band table above for N (LO multiple)		
Frequency read	dout accuracy (start, s	·		
			RBW + 2 Hz + 0.5 x horizontal resolution 1)	
Marker freque				
Accuracy		± (marker frequency x frequer	acy reference accuracy + 0.100 Hz)	
Delta counter acc	uracy	± (delta frequency x frequency	± (delta frequency x frequency reference accuracy + 0.141 Hz)	
Counter resolution	,	0.001 Hz	· · · · · ·	
	n (FFT and swept mod			
Range		<u>'</u>	imum frequency of instrument	
Resolution		2 Hz	<u> </u>	
Accuracy				
Swept		± (0.25 % x span + horizontal	resolution)	
FFT		± (0.10 % x span + horizontal resolution)		

<sup>1.</sup> Horizontal resolution is span/(sweep points -1).

Sweep time and triggering		
Range	Span = 0 Hz	1 μs to 6000 s
	Span ≥ 10 Hz	1 ms to 4000 s
Accuracy	Span ≥ 10 Hz, swept	± 0.01 % nominal
	Span ≥ 10 Hz, FFT	± 40 % nominal
	Span = 0 Hz	± 0.01 % nominal
Trigger	Free run, line, video, external 1, exte	·
Trigger Delay	Span = 0 Hz or FFT Span ≥ 10 Hz, swept	–150 to +500 ms 1 μs to 500 ms
	Resolution	0.1 μs
Time gating		
Gate methods	Gated LO; gated video; gated FFT	
Gate length range (except method = FFT)	100.0 ns to 5.0 s	
Gate delay range	0 to 100.0 s	
Gate delay jitter	33.3 ns p-p nominal	
Sweep (trace) point range		
All spans	1 to 40001	
Resolution bandwidth (RBW)		
Range (–3.01 dB bandwidth)	1 Hz to 3 MHz (10 % steps), 4, 5, 6,	8 MHz
Bandwidth accuracy (power)	1 Hz to 750 kHz	± 1.0 % (±0.044 dB)
	820 kHz to 1.2 MHz (< 3.6 GHz CF)	± 2.0 % (±0.088 dB)
	1.3 to 2 MHz (< 3.6 GHz CF) 2.2 to 3 MHz (< 3.6 GHz CF)	± 0.07 dB nominal ± 0.15 dB nominal
	4 to 8 MHz (< 3.6 GHz CF)	± 0.25 dB nominal
Bandwidth accuracy (-3.01 dB)		
RBW range	1 Hz to 1.3 MHz	± 2 % nominal
Selectivity (-60 dB/-3 dB)	4.1:1 nominal	
EMI bandwidth (CISPR compliant)	200 Hz, 9 kHz, 120 kHz, 1 MHz	(Option EMC or N6141A required)
EMI bandwidth (MIL STD 461E compliant)	10 Hz, 100 Hz, 1 kHz, 10 kHz,	(Option EMC or N6141A required)
A 1 - 1 - 1 - 1 - 1 - 1	100 kHz, 1 MHz	
Analysis bandwidth <sup>1</sup>		
Maximum bandwidth	Option B40 Option B25	40 MHz 25 MHz
	Standard	10 MHz
Video bandwidth (VBW)		
Range	1 Hz to 3 MHz (10 % steps), 4, 5, 6,	8 MHz, and wide open (labeled 50 MHz)
Accuracy	± 6 % nominal	
Measurement speed <sup>2</sup>	Standard	
Local measurement and display update rate	4 ms (250/s) nominal	
Remote measurement and LAN transfer rate	5 ms (200/s) nominal	
Marker peak search	1.5 ms nominal	
Center frequency tune and transfer (RF)	20 ms nominal	
Center frequency tune and transfer (µW)	47 ms nominal	
Measurement/mode switching	39 ms nominal	

<sup>1.</sup> Analysis bandwidth is the instantaneous bandwidth available around a center frequency over which the input signal can be digitized for further analysis or processing in the time, frequency, or modulation domain.

<sup>2.</sup> Sweep points = 101. Apply for instruments with S/N prefix ≥ MY/SG/US4910 or earlier instruments with Option PC2. Otherwise, refer to the MXA specification guide.

## Amplitude Accuracy and Range Specifications

Amplitude range			
Measurement range	Displayed average noise leve	el (DANL) to maximum sa	fe input level
Input attenuator range	0 to 70 dB in 2 dB steps		
Electronic attenuator (Option	EA3)		
Frequency range	20 Hz to 3.6 GHz		
Attenuation range Electronic attenuator range Full attenuation range (mechanical + electronic)	0 to 24 dB, 1 dB steps 0 to 94 dB, 1 dB steps		
Maximum safe input level			
Average total power (with and without preamp)	+30 dBm (1 W)		
Peak pulse power	$<$ 10 $\mu s$ pulse width, $<$ 1 $\%$ d	uty cycle +50 dBm (100 V	V) and input attenuation ≥ 30 dB
DC volts DC coupled AC coupled	± 0.2 Vdc ± 100 Vdc		
Display range			
Log scale	0.1 to 1 dB/division in 0.1 dE 1 to 20 dB/division in 1 dB s	•	)
Linear scale	10 divisions		
Scale units	dBm, dBmV, dBμV, dBmA, dB	ΒμΑ, V, W, A	
Frequency response		Specification	95th percentile (≈ 2σ)
(10 dB input attenuation, 20 to 30 °	C, preselector centering applied,	$\sigma$ = nominal standard dev	viation)
	20 kHz to 10 MHz 10 MHz <sup>1</sup> to 3.6 GHz 3.5 to 8.4 GHz 8.3 to 13.6 GHz 13.5 to 22.0 GHz 22.0 to 26.5 GHz	± 0.6 dB ± 0.45 dB ± 1.5 dB ± 2.0 dB ± 2.0 dB ± 2.5 dB	± 0.28 dB ± 0.17 dB ± 0.48 dB ± 0.47 dB ± 0.52 dB ± 0.71 dB
Preamp on (0 dB attenuation) <sup>2</sup>	100 kHz to 3.6 GHz 3.5 to 8.4 GHz 8.3 to 13.6 GHz 13.5 to 17.1 GHz 17.0 to 22.0 GHz 22.0 to 26.5 GHz	± 0.75 dB ± 2.0 dB ± 2.3 dB ± 2.5 dB ± 2.5 dB ± 3.5 dB	± 0.28 dB ± 0.67 dB ± 0.73 dB ± 0.97 dB ± 1.36 dB ± 1.48 dB

<sup>1.</sup> DC coupling required to meet specifications below 50 MHz. With AC coupling, specifications apply at frequencies of 50 MHz and higher. Statistical observations at 10 MHz with AC coupling show that most instruments meet the DC-coupled specifications, however, a small percentage of instruments are expected to have errors exceeding 0.5 dB at 10 MHz at the temperature extreme. The effect at 20 to 50 MHz is negligible but not warranted.

<sup>2.</sup> Apply for instruments with S/N prefix  $\geq$  MY/SG/US5051. For older instruments, refer to the MXA Specification Guide.

Input attenuation switching unco	ertainty	Specifications	Additional information
Attenuation > 2 dB , preamp off Relative to 10 dB	50 MHz (reference frequency) 20 Hz to 3.6 GHz	± 0.20 dB	± 0.08 dB typical ± 0.3 dB nominal
(reference setting)	3.5 to 8.4 GHz		± 0.5 dB nominal
	8.3 to 13.6 GHz 13.5 to 26.5 GHz		± 0.7 dB nominal ± 0.7 dB nominal
Total absolute amplitude accurac	су		
	$z \le RBW \le 1$ MHz, input signal $-10$ t ce level, any scale, $\sigma =$ nominal standard		auto-coupled except
	At 50 MHz	± 0.33 dB	
	At all frequencies 20 Hz to 3.6 GHz	± (0.33 dB + frequen ± 0.23 dB (95th Perc	, , ,
Preamp on	At all frequencies	± (0.39 dB + frequen	<u> </u>
Input voltage standing wave rati	o (VSWR) (≥ 10 dB input attenua	tion)	
	10 MHz to 3.6 GHz	< 1.2:1 nominal	
	3.6 to 8.4 GHz 8.4 to 13.6 GHz	< 1.5:1 nominal < 1.6:1 nominal	
	13.6 to 26.5 GHz	< 1.9:1 nominal	
Preamp on	10 MHz to 3.6 GHz	< 1.7:1 nominal	
(0 dB attenuation)	3.6 to 8.4 GHz	< 1.8:1 nominal	
	8.4 to 13.6 GHz 13.6 to 26.5 GHz	< 2.0:1 nominal < 2.0:1 nominal	
Resolution handwidth switching	uncertainty (referenced to 30 kHz		
1 Hz to 1.5 MHz RBW	± 0.05 dB	z novy	
1.6 MHz to 3 MHz RBW	± 0.10 dB		
4, 5, 6, 8 MHz RBW	± 1.0 dB		
Reference level			
Range			
Log scale	-170 to +30 dBm in 0.01 dB step	S	
Linear scale Accuracy	Same as Log (707 pV to 7.07 V) 0 dB		
•			
Display scale switching uncertain Switching between linear and log	0 dB		
Log scale/div switching	0 dB		
	0 UB		
Display scale fidelity	+ 0.10 dD +-+-!		
Between –10 dBm and –80 dBm input mixer level	± 0.10 dB total		
Trace detectors			
Normal, peak, sample, negative pea	k, log power average, RMS average,	and voltage average	
Preamplifier			
Frequency range	Option P03	100 kHz to 3.6 GHz	
	Option P08	100 kHz to 8.4 GHz	
	Option P13 Option P26	100 kHz to 13.6 GHz 100 kHz to 26.5 GHz	
Gain	100 kHz to 3.6 GHz	+20 dB nominal	
	3.6 to 26.5 GHz	+35 dB nominal	
Noise figure	100 kHz to 3.6 GHz	11 dB nominal	
	3.6 to 8.4 GHz 8.4 to 13.6 GHz	9 dB nominal 10 dB nominal	
	13.6 to 26.5 GHz	15 dB nominal	

# **Dynamic Range Specifications**

1 dB gain compression (two	-tone)	Total power at i	nput mixer
	20 to 500 MHz	0 dBm	+3 dBm nominal
	500 MHz to 3.6 GHz	3 dBm	+7 dBm nominal
	3.6 to 26.5 GHz	0 dBm	+4 dBm nominal
Preamp on	10 MHz to 3.6 GHz		–10 dBm nominal
(Option P03, P08, P13, P26)	3.6 to 26.5 GHz		To abili nominal
(0)110111 00, 1 00, 1 10, 1 20,	Tone spacing 100 kHz to 20 M	IH <sub>7</sub>	–26 dBm nominal
	Tone spacing > 70 MHz		–16 dBm nominal
Displayed average noise leve			
	ge detector, averaging type = Log, (	O dB input attenuation	n. IF Gain = High. 20 to 30 °C)
(,	g,gg -,p- =-9, .	Specification	Typical
	9 kHz to 1 MHz	•	
	1 to 10 MHz	-150 dBm	–153 dBm
	10 MHz to 2.1 GHz	–151 dBm	–154 dBm
	2.1 to 3.6 GHz	–149 dBm	–152 dBm
	3.6 to 8.4 GHz	–149 dBm	–153 dBm
	8.4 to 13.6 GHz	–148 dBm	–151 dBm
	13.6 to 17.1 GHz	–134 dBm	–147 dBm
	17.1 to 20.0 GHz	-133 dBm	–146 dBm
	20.0 to 26.5 GHz	-136 dBm	–142 dBm
Preamp on	100 kHz to 1 MHz		–149 dBm nominal
(Option P03, P08, P13, P26)	1 to 10 MHz	-161 dBm	–163 dBm
, , , , , ,	10 MHz to 2.1 GHz	-163 dBm	–166 dBm
	2.1 to 3.6 GHz	-162 dBm	–164 dBm
	3.6 to 8.4 GHz	-162 dBm	–166 dBm
	8.4 to 13.6 GHz	-162 dBm	–165 dBm
	13.6 to 17.1 GHz	-159 dBm	–163 dBm
	17.1 to 20.0 GHz	-157 dBm	–161 dBm
	20.0 to 26.5 GHz	-152 dBm	–157 dBm
Spurious responses			
Residual responses (Input ter-	200 kHz to 8.4 GHz (swept)	–100 dBm	
minated and 0 dB attenuation)	Zero span or FFT or other	-100 dBm nomin	al
	frequencies		
Image responses	10 MHz to 3.6 GHz	-80 dBc (-107 dE	Bc typical)
	3.6 to 13.6 GHz	-78 dBc (-88 dBc	
	13.6 to 17.1 GHz	-74 dBc (-85 dBc	
	17.1 to 22 GHz	-70 dBc (-82 dBc	
	22 to 26.5 GHz	-68 dBc (-78 dBc	
LO related spurious	10 MHz to 3.6 GHz	-90 dBc + 20xlog	gN¹ typical
(f > 600 MHz from carrier)			• ••
Other spurious			
f ≥ 10 MHz from carrier	-80 dBc + 20xlogN <sup>1</sup>		

<sup>1.</sup> N is the LO multiplication factor.

0 11 11 11 11 11 11 11				
Second harmonic distortion (SHI)				
	Source frequency	Mixer level	Distortion	SHI
	10 MHz to 1.25 GHz	–15 dBm	-60 dBc	+45 dBm
	1.25 to 1.8 GHz	-15 dBm	–56 dBm	+41 dBm
	1.75 to 7 GHz	-15 dBm	-80 dBc	+65 dBm
	7 to 11 GHz	-15 dBm	-70 dBc	+55 dBm
	11 to 13.25 GHz	–15 dBm	-65 dBc	+50 dBm
		Preamp level	Distortion	SHI
Preamp on	10 MHz to 1.8 GHz	–45 dBm	–78 dBc nominal	+33 dBm nominal
(Option P03, P08, P13, P26)	1.8 to 13.25 GHz	–50 dBm	-60 dBc nominal	+10 dBm nominal
Third-order intermodulation dis	tortion (TOI)			
(Two –30 dBm tones at input mixer wi for IF prefilter bandwidths)	th tone separation > 5 time	s IF prefilter bandwidth,	20 to 30 °C, see Speci	fications Guide
		Distortion	TOI	TOI (typical)
	10 to 100 MHz	-84 dBc	+12 dBm	+17 dBm
	100 to 400 MHz	-90 dBc	+15 dBm	+20 dBm
	400 MHz to 1.7 GHz	-92 dBc	+16 dBm	+20 dBm
	1.7 to 3.6 GHz	-92 dBc	+16 dBm	+19 dBm
	3.6 to 8.4 GHz	–90 dBc	+15 dBm	+18 dBm
	8.4 to 13.6 GHz	-90 dBc	+15 dBm	+18 dBm
	13.6 to 26.5 GHz	-80 dBc	+10 dBm	+14 dBm
D ΔΓ JD 4	10 to 500 MHz	-98 dBc nominal		. 4 . ID
Preamp on (two –45 dBm tones at	10 10 300 101112	-30 ubc Hollillai		+4 dBm nominal
preamp input)	500 MHz to 3.6 GHz	–100 dBc nominal		+4 dBm nominal +5 dBm nominal

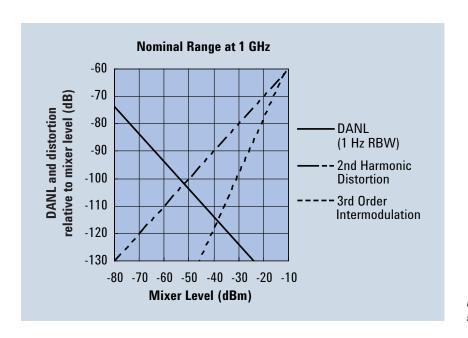


Figure 1. Nominal dynamic range — Band 0, for second and third order distortion, 20 Hz to 3.6 GHz

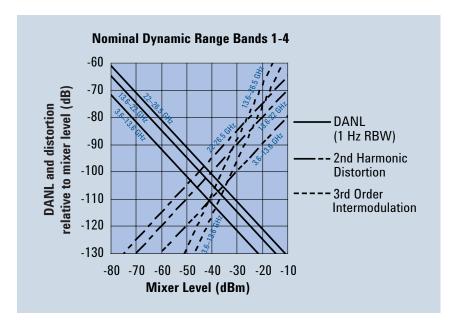


Figure 2. Nominal dynamic range – Bands 1 to 4, for second and third order distortion, 3.6 GHz to 26.5 GHz

Phase noise 1	Offset	Specification	Typical
Noise sidebands	100 Hz	−84 dBc/Hz	−88 dBc/Hz
(20 to 30 °C, CF = 1 GHz)	1 kHz		-101 dBc/Hz nominal
	10 kHz	−103 dBc/Hz	-106 dBc/Hz
	100 kHz	−115 dBc/Hz	-117 dBc/Hz
	1 MHz	−135 dBc/Hz	-137 dBc/Hz
	10 MHz		-148 dBc/Hz nominal

<sup>1.</sup> For nominal values, refer to Figure 3.

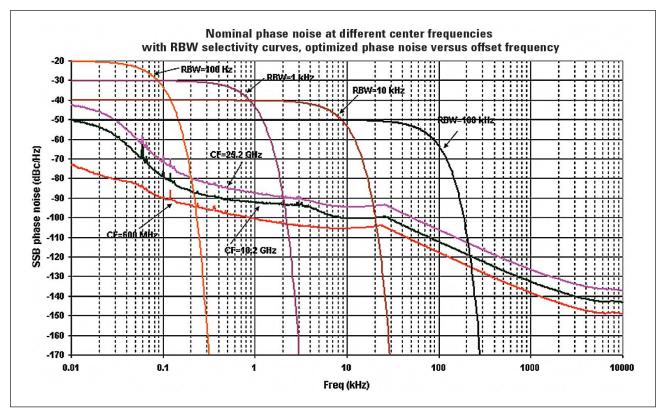


Figure 3. Nominal phase noise at different center frequencies

# PowerSuite Measurement Specifications

Channel power			
Amplitude accuracy, W-CDMA or IS95 (20 to 30 °C, attenuation = 10 dB)	± 0.80 dB (± 0.30 d	IB 95th percentile)	
Occupied bandwidth			
Frequency accuracy	± [span/1000] non	ninal	
Adjacent channel power			
Accuracy, W-CDMA (ACLR) (at specific mixer levels and ACLR ranges)	Adjacent	Alternate	
MS BTS	± 0.14 dB ± 0.49 dB	± 0.21 dB ± 0.44 dB	
Dynamic range (typical) Without noise correction With noise correction	–73 dB –78 dB	–79 dB –82 dB	
Offset channel pairs measured	1 to 6		
ACP measurement and transfer time (fast method)	14 ms nominal (σ =	= 0.2 dB)	
Multiple number of carriers measured	Up to 12		
Power statistics CCDF			
Histogram resolution	0.01 dB		
Harmonic distortion			
Maximum harmonic number	10th		
Result	Fundamental power (dBm), relative harmonics power (dBc), total harmonic distortion in %		
Intermod (TOI)	Measure the third-order products and intercepts from two tones		
Burst power			
Methods	Power above thres	hold, power within burst width	
Results	Single burst output within burst, burst	t power, average output power, maximum power, minimum power width	
Spurious emission			
W-CDMA (1 to 3.6 GHz) table-driven spuriou	ıs signals; search acros	ss regions	
Dynamic range Absolute sensitivity	96.7 dB -84.4 dBm	(101.7 dB typical) (–89.4 dBm typical)	
Spectrum emission mask (SEM)			
cdma2000® (750 kHz offset) Relative dynamic range (30 kHz RBW) Absolute sensitivity Relative accuracy	78.9 dB -99.7 dBm ± 0.11 dB	(85.0 dB typical) (–104.7 dBm typical)	
3GPP W-CDMA (2.515 MHz offset) Relative dynamic range (30 kHz RBW) Absolute sensitivity Relative accuracy	81.9 dB -99.7 dBm ± 0.12 dB	(88.2 dB typical) (–104.7 dBm typical)	

## **General Specifications**

### Temperature range

Operating 0 to 55 °C Storage -40 to 65 °C

### **EMC**

Complies with European EMC Directive 2004/108/EC

- IEC/EN 61326-1 or IEC/EN 61326-2-1
- · CISPR Pub 11 Group 1, class A
- AS/NZS CISPR 11:2002
- ICES/NMB-001

This ISM device complies with Canadian ICES-001

Cet appareil ISM est conforme à la norme NMB-001 du Canada

#### Safety

Complies with European Low Voltage Directive 73/23/EEC, amended by 93/68/EEC

- IEC/EN 61010-1 2nd Edition
- Canada: CSA C22.2 No. 61010-1
- USA: UL 61010-1 2nd Edition

Audio noise	
Acoustic noise emission	Geraeuschemission
LpA < 70 dB	LpA < 70 dB
Operator position	Am Arbeitsplatz
Normal position	Normaler Betrieb
Per ISO 7779	Nach DIN 45635 t.19

### **Environmental stress**

Samples of this product have been type tested in accordance with the Agilent Environmental Test Manual and verified to be robust against the environmental stresses of storage, transportation, and end-use; those stresses include, but are not limited to, temperature, humidity, shock, vibration, altitude, and power line conditions; test methods are aligned with IEC 60068-2 and levels are similar to MILPRF-28800F Class 3.

Power requirements	
Voltage and frequency (nominal)	100 to 120 V, 50/60/400 Hz 220 to 240 V, 50/60 Hz
Power consumption On Standby	390 W maximum 20 W
Display	
Resolution Size	1024 x 768, XGA 213 mm (8.4 in.) diagonal (nominal)
Data storage	
Internal External	> = 80 GB nominal (removable solid state drive) Supports USB 2.0 compatible memory devices
Weight (without options)	
Net Shipping	16 kg (35 lbs) nominal 28 kg (62 lbs) nominal
Dimensions	
Height Width Length	177 mm (7.0 in) 426 mm (16.8 in) 368 mm (14.5 in)
Warranty	

#### vvarranty

The MXA signal analyzer is supplied with a one-year warranty

### Calibration cycle

The recommended calibration cycle is two years; calibration services are available through Agilent service centers

## Inputs and Outputs

Front panel	
RF input	
Connector	Type-N female, 50 $\Omega$ nominal
Analog baseband IQ inputs (Option BBA/S40) <sup>1</sup> Connectors (I, Q, I-Bar, Q-Bar, and Cal Out)	BNC female
Cal Out	
Signal	AC coupled square wave
Frequency	Selectable between 1 kHz and 250 kHz
Input impedance (4 connectors: I, Q, I-, Q-)	50 $\Omega$ , 1 M $\Omega$ (selectable, nominal)
Probes supported <sup>2</sup>	1100 A 1101 A 1100 A 1104 A
Active probe Passive probe	1130A, 1131A, 1132A, 1134A 1161A
Input return loss	-35 dB (0 to 10 MHz, nominal)
50 Ω impedance only selected	–30 dB (10 to 40 MHz. nominal)
Probe power	,
Voltage/current	+15 Vdc, $\pm 7~\%$ at 150 mA max nominal
	$-12.6~\text{Vdc}$ , $\pm 10~\%$ at 150 mA max nominal
USB 2.0 ports	
Master (2 ports)	Compatible with HCD 2.0
Standard Connector	Compatible with USB 2.0 USB Type-A female
Output current	0.5 A nominal
Rear panel	
10 MHz out	
Connector	BNC female, 50 $\Omega$ nominal
Connector Output amplitude	≥ 0 dBm nominal
Connector Output amplitude Frequency	
Connector Output amplitude Frequency Ext Ref In	≥ 0 dBm nominal 10 MHz ± (10 MHz x frequency reference accuracy)
Connector Output amplitude Frequency Ext Ref In Connector	$\geq$ 0 dBm nominal 10 MHz $\pm$ (10 MHz x frequency reference accuracy) BNC female, 50 $\Omega$ nominal
Connector Output amplitude Frequency  Ext Ref In Connector Input amplitude range	≥ 0 dBm nominal 10 MHz ± (10 MHz x frequency reference accuracy)
Connector Output amplitude Frequency Ext Ref In Connector	$\geq$ 0 dBm nominal 10 MHz $\pm$ (10 MHz x frequency reference accuracy) BNC female, 50 $\Omega$ nominal $-5$ to 10 dBm nominal
Connector Output amplitude Frequency  Ext Ref In Connector Input amplitude range Input frequency Frequency lock range  Trigger 1 and 2 inputs	≥ 0 dBm nominal 10 MHz ± (10 MHz x frequency reference accuracy)  BNC female, 50 Ω nominal -5 to 10 dBm nominal 1 to 50 MHz nominal ± 5 x 10 <sup>-6</sup> of specified external reference input frequency
Connector Output amplitude Frequency  Ext Ref In Connector Input amplitude range Input frequency Frequency lock range  Trigger 1 and 2 inputs Connector	≥ 0 dBm nominal 10 MHz ± (10 MHz x frequency reference accuracy)  BNC female, 50 Ω nominal -5 to 10 dBm nominal 1 to 50 MHz nominal ± 5 x 10 <sup>-6</sup> of specified external reference input frequency  BNC female
Connector Output amplitude Frequency  Ext Ref In Connector Input amplitude range Input frequency Frequency lock range  Trigger 1 and 2 inputs Connector Impedance	$\geq 0 \text{ dBm nominal}$ $10 \text{ MHz} \pm (10 \text{ MHz} \times \text{frequency reference accuracy})$ BNC female, $50 \Omega$ nominal $-5 \text{ to } 10 \text{ dBm nominal}$ $1 \text{ to } 50 \text{ MHz nominal}$ $\pm 5 \times 10^{-6} \text{ of specified external reference input frequency}$ BNC female $> 10 \text{ k}\Omega \text{ nominal}$
Connector Output amplitude Frequency  Ext Ref In Connector Input amplitude range Input frequency Frequency lock range  Trigger 1 and 2 inputs Connector Impedance Trigger level range	≥ 0 dBm nominal 10 MHz ± (10 MHz x frequency reference accuracy)  BNC female, 50 Ω nominal -5 to 10 dBm nominal 1 to 50 MHz nominal ± 5 x 10 <sup>-6</sup> of specified external reference input frequency  BNC female
Connector Output amplitude Frequency  Ext Ref In Connector Input amplitude range Input frequency Frequency lock range  Trigger 1 and 2 inputs Connector Impedance Trigger level range  Trigger 1 and 2 outputs	$\geq 0 \text{ dBm nominal}$ $10 \text{ MHz} \pm (10 \text{ MHz} \times \text{frequency reference accuracy})$ BNC female, $50 \Omega$ nominal $-5 \text{ to } 10 \text{ dBm nominal}$ $1 \text{ to } 50 \text{ MHz nominal}$ $\pm 5 \times 10^{-6} \text{ of specified external reference input frequency}$ BNC female $> 10 \text{ k}\Omega \text{ nominal}$ $-5 \text{ to } 5 \text{ V}$
Connector Output amplitude Frequency  Ext Ref In Connector Input amplitude range Input frequency Frequency lock range  Trigger 1 and 2 inputs Connector Impedance Trigger level range  Trigger 1 and 2 outputs Connector	$\geq 0 \text{ dBm nominal}$ $10 \text{ MHz} \pm (10 \text{ MHz} \times \text{frequency reference accuracy})$ $BNC \text{ female, } 50 \Omega \text{ nominal}$ $-5 \text{ to } 10 \text{ dBm nominal}$ $1 \text{ to } 50 \text{ MHz nominal}$ $\pm 5 \times 10^{-6} \text{ of specified external reference input frequency}$ $BNC \text{ female}$ $> 10 \text{ k}\Omega \text{ nominal}$ $-5 \text{ to } 5 \text{ V}$ $BNC \text{ female}$
Connector Output amplitude Frequency  Ext Ref In Connector Input amplitude range Input frequency Frequency lock range  Trigger 1 and 2 inputs Connector Impedance Trigger level range  Trigger 1 and 2 outputs	$\geq 0 \text{ dBm nominal}$ $10 \text{ MHz} \pm (10 \text{ MHz} \times \text{frequency reference accuracy})$ BNC female, $50 \Omega$ nominal $-5 \text{ to } 10 \text{ dBm nominal}$ $1 \text{ to } 50 \text{ MHz nominal}$ $\pm 5 \times 10^{-6} \text{ of specified external reference input frequency}$ BNC female $> 10 \text{ k}\Omega \text{ nominal}$ $-5 \text{ to } 5 \text{ V}$
Connector Output amplitude Frequency  Ext Ref In Connector Input amplitude range Input frequency Frequency lock range  Trigger 1 and 2 inputs Connector Impedance Trigger level range  Trigger 1 and 2 outputs Connector Impedance Impedance Trigger 1 and 2 outputs Connector Impedance	$\geq 0 \text{ dBm nominal}$ $10 \text{ MHz} \pm (10 \text{ MHz} \times \text{frequency reference accuracy})$ BNC female, $50 \Omega$ nominal $-5 \text{ to } 10 \text{ dBm nominal}$ $1 \text{ to } 50 \text{ MHz nominal}$ $\pm 5 \times 10^{-6} \text{ of specified external reference input frequency}$ BNC female $> 10 \text{ k}\Omega \text{ nominal}$ $-5 \text{ to } 5 \text{ V}$ BNC female $50 \Omega \text{ nominal}$
Connector Output amplitude Frequency  Ext Ref In Connector Input amplitude range Input frequency Frequency lock range  Trigger 1 and 2 inputs Connector Impedance Trigger level range  Trigger 1 and 2 outputs Connector Impedance Level  Monitor output Connector	$\geq 0 \text{ dBm nominal} \\ 10 \text{ MHz} \pm (10 \text{ MHz} \times \text{frequency reference accuracy}) \\ \\ \text{BNC female, } 50 \Omega \text{ nominal} \\ -5 \text{ to } 10 \text{ dBm nominal} \\ 1 \text{ to } 50 \text{ MHz nominal} \\ \pm 5 \times 10^{-6} \text{ of specified external reference input frequency} \\ \\ \text{BNC female} \\ > 10 \text{ k}\Omega \text{ nominal} \\ -5 \text{ to } 5 \text{ V} \\ \\ \text{BNC female} \\ 50 \Omega \text{ nominal} \\ 5 \text{ V TTL nominal} \\ \\ \text{VGA compatible, } 15\text{-pin mini D-SUB} \\ \\$
Connector Output amplitude Frequency  Ext Ref In Connector Input amplitude range Input frequency Frequency lock range  Trigger 1 and 2 inputs Connector Impedance Trigger level range  Trigger 1 and 2 outputs Connector Impedance Level  Monitor output	$\geq 0 \text{ dBm nominal} \\ 10 \text{ MHz} \pm (10 \text{ MHz} \times \text{frequency reference accuracy}) \\ \\ \text{BNC female, } 50 \Omega \text{ nominal} \\ -5 \text{ to } 10 \text{ dBm nominal} \\ 1 \text{ to } 50 \text{ MHz nominal} \\ \pm 5 \times 10^{-6} \text{ of specified external reference input frequency} \\ \\ \text{BNC female} \\ > 10 \text{ k}\Omega \text{ nominal} \\ -5 \text{ to } 5 \text{ V} \\ \\ \text{BNC female} \\ 50 \Omega \text{ nominal} \\ 5 \text{ V TTL nominal} \\ \\ \end{cases}$

<sup>1.</sup> For additional specifications, please refer to the MXA Signal Analyzer Option BBA: Analog Baseband IQ Inputs Technical Overview, literature number 5989-6538EN.

<sup>2.</sup> For more details, please refer to the Agilent Probe Configuration Guides, literature numbers 5968-7141EN and 5989-6162EN; probe heads are necessary to attach to your device properly and probe connectivity kits such as E2668B, E2669A. or E2675A are required.

Rear panel	
Noise source drive +28 V (pulsed)	
Connector	BNC female
SNS Series noise source	
Anolog out	
Connector	BNC female (used by Option YAS)
USB 2.0 ports	
Master (4 ports) Standard	Compatible with USB 2.0
Connector	USB Type-A female
Output current	0.5 A nominal
Slave (1 port)	
Standard	Compatible with USB 2.0
Connector	USB Type-B female
Output current	0.5 A nominal
GPIB interface Connector	IEEE-488 bus connector
GPIB codes	SH1, AH1, T6, SR1, RL1, PP0, DC1, C1, C2, C3, C28, DT1, L4, C0
GPIB mode	Controller or device
LAN TCP/IP interface	
Standard	1000Base-T
Connector	RJ45 Ethertwist
IF output	
Connector	SMA female, shared by Option CR3 and CRP
Impedance	50 Ω nominal
Wideband IF output, Option CR3	
Center frequency	222 E MIL-
SA mode or I/Q analyzer with IF BW $\leq$ 25 MHz with Option B40	322.5 MHz 250 MHz
Conversion gain	-1 to +4 dB (nominal) plus RF frequency response
Bandwidth	T to 1 ab (nonlinar) place in requestoy recipolise
Low band	Up to 140 MHz (nominal)
High band, with preselector	Depends on center frequency
High band, with preselector bypassed <sup>1</sup>	Up to 500 MHz
Programmable IF output, Option CRP	
Center frequency	
Range	10 to 75 MHz (user selectable)
Resolution	0.5 MHz
Conversion gain	-1 to +4 dB (nominal) plus RF frequency response
Bandwidth	400 100 1
Output at 70 MHz	100 MHz (nominal)
Low band or high band with preselector bypassed <sup>1</sup> Preselected band	Depends on RF center frequency
Lower output frequencies	Subject to folding
Residual output signals	≤ -88 dBm (nominal)
Ontion MPB installed and enabled	

<sup>1.</sup> Option MPB installed and enabled.

## I/Q Analyzer

Resolution bandwidth (spectrum measurer	nent)			
Range Overall Span = 1 MHz Span = 10 kHz Span = 100 Hz	100 mHz to 3 M 50 Hz to 1 MHz 1 Hz to 10 kHz 100 mHz to 100			
Window shapes				
Flat top, Uniform, Hanning, Gaussian, Blackman, Bla	ckman-Harris, Kaise	er Bessel (K-B 70 dB	, K-B 90 dB and K-B	110 dB)
Analysis bandwidth				
Standard instrument Option B25 Option B40	10 Hz to 10 MH 10 Hz to 25 MH 10 Hz to 40 MH	Z		
IF frequency response (standard 10 MHz IF	<u> </u>			
IF frequency response (demodulation and FFT response)			•	
Center frequency (GHz)	Span (MHz)	Preselector	Max. error	RMS (nominal)
$\leq 3.6$ 3.6 $< f \leq 26.5$ 3.6 $< f \leq 26.5$	≤ 10 ≤ 10 ≤ 10	n/a on off <sup>1</sup>	± 0.40 dB ± 0.45 dB	0.04 dB 0.25 dB 0.04 dB
IF phase linearity (deviation from mean pha	ase linearity, non	ninal)		
Center frequency (GHz)	Span (MHz)	Preselector	Peak-to-peak	RMS
$\leq 3.6$ 3.6 < f \le 26.5 3.6 < f \le 26.5	≤ 10 ≤ 10 ≤ 10	n/a on off <sup>1</sup>	± 0.5° ± 1.5° ± 0.5°	0.2° 0.4° 0.2°
Data acquisition (10 MHz IF path)				
Time record length IQ analyzer	4,000,000 IQ sa	mple pairs		
89600 VSA software or N9064A VXA	32-bit packing	64-bit packing		Memory
Option DP2, B40 or MPB None of the above	536 MSa 62.5 MSa	268 MSa 31.25 MSa		2 GB 256 MB
Sample rate Option DP2, B40 or MPB None of the above	100 MSa/s 90 MSa/s			
ADC resolution Option DP2, B40 or MPB None of the above	16 bits 14 bits			
Option B25 25 MHz analysis bandwidth				
IF frequency response (B25 IF path)				
IF frequency response (demodulation and FFT response	nse relative to the c	enter frequency, 20	to 30 °C)	
Center frequency (GHz)	Span (MHz)	Preselector	Max. error	RMS (nominal)
$\leq 3.6$ 3.6 < f $\leq 26.5$ 3.6 < f $\leq 26.5$	$10 \text{ to } \le 25$ $10 \text{ to } \le 25$ $10 \text{ to } \le 25$	n/a on off <sup>1</sup>	± 0.45 dB ± 0.45 dB	0.051 dB 0.45 dB 0.05 dB

<sup>1.</sup> Option MPB is installed and enabled.

IF phase linearity (deviation from me	an phase linearit	y, nominal)		
Center frequency (GHz)	Span (MHz)	Preselector	Peak-to-peak	RMS
0.02 ≤ f < 3.6	≤ 25	n/a	± 0.5 °	0.2 °
$3.6 \le f \le 26.5$	≤ 25	on	± 1.5 °	0.4 °
$3.6 \le f \le 26.5$	≤ 25	off <sup>1</sup>	± 0.5 °	0.2 °
Data acquisition (B25 IF path)				
Time record length (IQ pairs) IQ Analyzer	4,000,000 IQ sam	nla naira		
89600 software or N9064A	32-bit packing	64-bit packing		Memory
Option DP2, B40 or MPB	536 MSa	268 MSa		2 GB
None of the above	62.5 MSa	31.25 MSa		256 MB
Sample rate	02.004	0.1.20 11.00		
Option DP2, B40 or MPB	100 MSa/s			
None of the above	90 MSa/s			
ADC resolution				
Option DP2, B40 or MPB None of the above	16 bits 14 bits			
Option B40 40 MHz analysis bandwid				
IF frequency response (B40 IF path)	ıtıı			
	T 100 0		20 ( 20 00)	
IF frequency response (demodulation and FF	·	•	<u> </u>	D140 /
Center frequency (GHz)	Span (MHz)	Preselector	Max. error	RMS (nominal)
0.03 ≤ f < 3.6 3.6 ≤ f ≤26.5	≤ 40 ≤ 40	n/a off <sup>1</sup>	± 0.3 dB ± 0.25 dB	± 0.08 dB ± 0.08 dB
IF phase linearity (deviation from mean phase		011	± 0.20 ub	± 0.00 UD
·		Duncalantar	Dook to mook	DMC
Center frequency (GHz)	Span (MHz)	Preselector	Peak-to-peak	RMS
$0.02 \le f < 3.6$ $3.6 \le f \le 26.5$	40 40	n/a off <sup>1</sup>	0.3 ° nominal 0.7 ° nominal	0.06 ° nominal 0.17 ° nominal
Dynamic range (B40 IF path)	40	OII	0.7 Homman	0.17 Hollillal
SFDR (Spurious-free dynamic range)				
Signal frequency within ± 12 MHz of	–77 dBc nominal			
center	-// ubc nonnia			
Signal frequency anywhere within analysis B	W			
Spurious response within ± 18 MHz of center	-74 dBc nominal			
Response anywhere within analysis BW	-74 dBc nominal			
Data acquisition (B40 IF path)		ifications	Supplemental i	nformation
Time record length (IQ pairs)	<del>_</del> <del>o</del> pcc	- Insuriorio	ouppromoneur	morniacioni
IQ Analyzer	4,000,000 sample	s (I/Q pairs)		
89600 VSA software or N9064A VXA	32-bit packing	64-bit packing		
Length (IQ sample pairs) Length (time units)	536 MSa	268 MSa	2 GB total memory Samples/(Span x	
Sample rate			. , ,	
At ADC	200 Msa/s			
IQ pairs	10 6:4-		Span x 1.28	
ADC resolution	12 bits			

<sup>1.</sup> Option MPB is installed and enabled.

### **Related Literature**

### Agilent MXA signal analyzers

Brochure	5989-5047EN
Configuration guide	5989-4943EN

For more information or literature resources please visit the web: www.agilent.com/find/mxa



### Agilent Email Updates

www.agilent.com/find/emailupdates
Get the latest information on the
products and applications you select.



### www.lxistandard.org

LAN eXtensions for Instruments puts the power of Ethernet and the Web inside your test systems. Agilent is a founding member of the LXI consortium.

### **Agilent Channel Partners**

www.agilent.com/find/channelpartners
Get the best of both worlds: Agilent's
measurement expertise and product
breadth, combined with channel
partner convenience.



Agilent Advantage Services is committed to your success throughout your equipment's lifetime. We share measurement and service expertise to help you create the products that change our world. To keep you competitive, we continually invest in tools and processes that speed up calibration and repair, reduce your cost of ownership, and move us ahead of your development curve.

www.agilent.com/find/advantageservices



www.agilent.com/quality

cdma2000® is a registered certification mark of the Telecommunications Industry Association. Used under license.

Windows® and MS Windows are U.S. registered trademarks of Microsoft® Corporation.

### www.agilent.com

For more information on Agilent Technologies' products, applications or services, please contact your local Agilent office. The complete list is available at:

### www.agilent.com/find/contactus

#### **Americas**

Canada	(877) 894 4414
Brazil	(11) 4197 3500
Mexico	01800 5064 800
United States	(800) 829 4444

#### **Asia Pacific**

Australia	1 800 629 485
China	800 810 0189
Hong Kong	800 938 693
India	1 800 112 929
Japan	0120 (421) 345
Korea	080 769 0800
Malaysia	1 800 888 848
Singapore	1 800 375 8100
Taiwan	0800 047 866
Other AP Countries	(65) 375 8100

### **Europe & Middle East**

Belgium	32 (0) 2 404 93 40
Denmark	45 70 13 15 15
Finland	358 (0) 10 855 2100
France	0825 010 700*
	*0.125 €/minute
Germany	49 (0) 7031 464 6333
Ireland	1890 924 204
Israel	972-3-9288-504/544
Italy	39 02 92 60 8484
Netherlands	31 (0) 20 547 2111
Spain	34 (91) 631 3300
Sweden	0200-88 22 55
United Kingdom	44 (0) 118 9276201

For other unlisted countries:

### www.agilent.com/find/contactus

Revised: October 14, 2010

Product specifications and descriptions in this document subject to change without notice.

© Agilent Technologies, Inc. 2010 Printed in USA, December 23, 2010 5989-4942EN

